


ANEXOS (ANNEXES) al documento de depósito de la línea iPSC SYS FiPS135

ANEXO 1: Análisis de microsatelites


ANNEX 1: Microsatellite analysis

STR	Size range	iPSC	Fibroblast
AMEL	104-112 bps	104/104	104/104
D13S317	166-204 bps	179/187	179/187
D16S539	258-310 bps	286/294	286/294
D18S51	279-364 bps	302/310	302/310
D21S11	195-262 bps	215/233	215/233
D3S1358	94-148 bps	132/132	132/132
D7S820	208-252 bps	224/232	224/232
D8S1179	198-252 bps	222/226	222/226
FGA	305-466 bps	333/349	333/349
Penta D	365-448 bps	418/427	418/427
Penta E	368-480 bps	418/428	418/428
TH01	148-194 bps	169/169	169/169
TPOX	255-303 bps	269/285	269/285
vWA	120-184 bps	150/154	150/154

ANEXO 2: Test de diferenciación *in vitro*
ANNEX 2: *in vitro differentiation test*

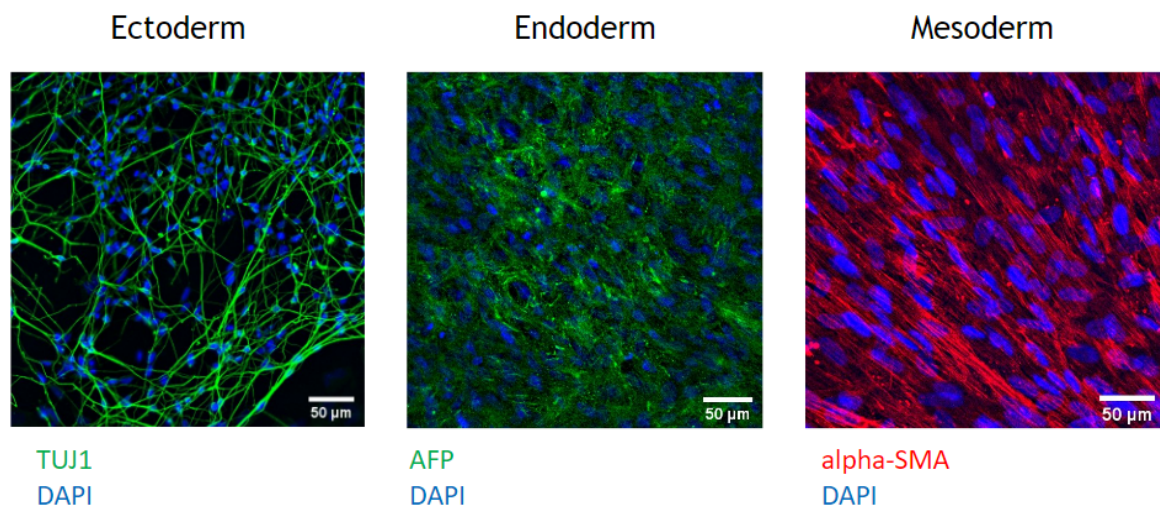

ANEXO 3: Cariotipo
ANNEX 3: *Karyotype*

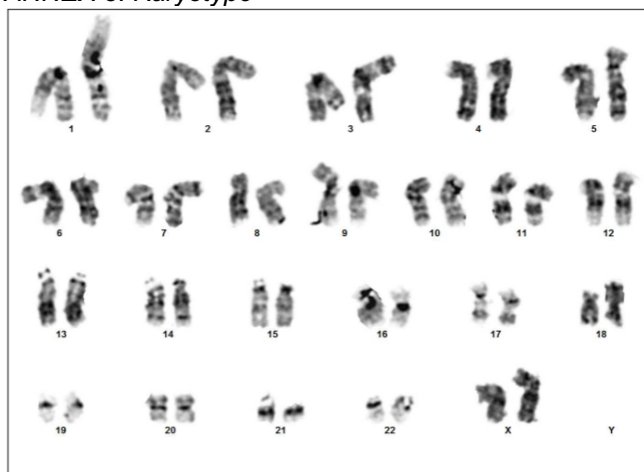

ANEXO 4: Test de micoplasma
ANNEX 4: *Mycoplasma test*

